

The Lexogen logo features the word "LEXOGEN" in a bold, sans-serif font. The letters "L", "E", and "X" are green, while "O", "G", "E", and "N" are dark blue. The background of the entire page is white with a pattern of semi-transparent, light blue spheres of various sizes and soft shadows, creating a molecular or network-like aesthetic.

LEXOGEN

Enabling complete transcriptome sequencing

RiBO COP™

Select and Deplete

rRNA Depletion Kit V1.3 User Guide

Catalog Number:
037 (RiboCop rRNA Depletion Kit V1.3 (Human/Mouse/Rat))
096 (CORALL Total RNA-Seq Library Prep Kit with RiboCop)



The RiboCop Protocol and User Guide Has Been Updated!

This User Guide features the new optimized V1.3 Protocol for RiboCop rRNA Depletion (Human/Mouse/Rat).

The V1.3 protocol reduces hands-on and overall preparation time, featuring:

- Less protocol steps for Bead Preparation and Purification
- Shorter incubation times for Depletion and Purification

The full list of updates for the V1.3 protocol are listed in the Revision History (see p.19).

The Conditioning Solution (**CS**) is no longer required for the V1.3 protocol. However, the provided RiboCop Kit components and component volumes (including **CS**) have not changed. Thus, the former V1.2 protocol can still be performed if required and full V1.2 protocol information is included in the User Guide (see p.14 – 17).

FOR RESEARCH USE ONLY. NOT INTENDED FOR DIAGNOSTIC OR THERAPEUTIC USE.

INFORMATION IN THIS DOCUMENT IS SUBJECT TO CHANGE WITHOUT NOTICE.

Lexogen does not assume any responsibility for errors that may appear in this document.

PATENTS AND TRADEMARKS

RiboCop™ is a trademark of Lexogen. Lexogen is a registered trademark (EU, CH, USA). RNasin® is a registered trademark of Promega Corporation. Bioanalyzer®, is a trademark of Agilent Technologies, Inc.. Qubit™, RNaseZap™, RNAlater®, and ERCC are registered trademarks of Ambion, Inc.. Thermomix® is a registered trademark of Eppendorf AG.

All other brands and names contained in this user guide are the property of their respective owners.

Lexogen does not assume responsibility for violations or patent infringements that may occur with the use of its products.

LIABILITY AND LIMITED USE LABEL LICENSE: RESEARCH USE ONLY

This document is proprietary to Lexogen. The RiboCop rRNA Depletion Kits are intended for use in research and development only. They need to be handled by qualified and experienced personnel to ensure safety and proper use. Lexogen does not assume liability for any damage caused by the improper use or the failure to read and explicitly follow this user guide. Furthermore, Lexogen does not assume warranty for merchantability or suitability of the product for a particular purpose.

The purchase of the product does not convey the right to resell, distribute, further sublicense, repackage, or modify the product or any of its components. This document and its contents shall not be used or distributed for any other purpose and/or otherwise communicated, disclosed, or reproduced in any way without the prior written consent of Lexogen.

For information on purchasing additional rights or a license for use other than research, please contact Lexogen.

WARRANTY

Lexogen is committed to providing excellent products. Lexogen warrants that the product performs to the standards described in this user guide until the expiration date. Should this product fail to meet these standards due to any reason other than misuse, improper handling, or storage, Lexogen will replace the product free of charge or issue a credit for the purchase price. Lexogen does not provide any warranty if product components are replaced with substitutes.

Under no circumstances shall the liability of this warranty exceed the purchase price of this product.

LITERATURE CITATION

When describing a procedure for publication using this product, please refer to it as the RiboCop rRNA Depletion Kit V1.3.

We reserve the right to change, alter, or modify any product without notice to enhance its performance.

CONTACT INFORMATION

Lexogen GmbH

Campus Vienna Biocenter 5
1030 Vienna, Austria
www.lexogen.com
E-mail: info@lexogen.com

Support

E-mail: support@lexogen.com
Tel. +43 (0) 1 3451212-41
Fax. +43 (0) 1 3451212-99

Table of Contents

1. Overview	4
2. Kit Components and Storage Conditions	6
3. User-Supplied Consumables and Equipment	7
4. Guidelines	8
5. Detailed Protocol - RiboCop V1.3	10
6. Short Procedure - RiboCop V1.3	13
7. Detailed Protocol - RiboCop V1.2	14
8. Short Procedure - RiboCop V1.2	17
9. Appendix A: RNA Requirements and Results	18
10. Appendix B: Downstream Processing.	19
11. Appendix C: Revision History.	19

1. Overview

Lexogen's RiboCop rRNA Depletion Kit enables removal of ribosomal RNA (rRNA) from human, mouse, and rat total RNA and is suited for Next Generation Sequencing (NGS) and similar applications.

Samples are treated using a set of affinity probes for specific depletion of rRNA sequences. The number and positioning of probes are designed for compatibility with intact and fragmented input RNA. RiboCop probes efficiently remove ribosomal RNA and therefore afford a comprehensive view of transcriptome composition. Samples void of 28S, 18S, 5.8S, 45S, 5S, mt16S, and mt12S ribosomal sequences are obtained within 2 hours of total processing time. No enzymatic reactions or mechanical shearing steps are involved, leaving full-length transcripts intact for downstream processing.

Affinity probes are mixed with total RNA are mixed and denatured, facilitating access of probes to target sequences. Afterwards, hybridization is performed at elevated temperature. Depletion beads are conditioned and used to remove probes that are hybridized to ribosomal RNA from the solution. A final purification step using magnetic beads rounds off the procedure. Recovered RNA may be directly used for NGS library preparation, with sufficient volume for optional quality control. The entire protocol is automation-friendly, using magnetic beads for depletion and purification purposes.

The recommended input range for RiboCop is 1 - 1,000 ng of total RNA. RiboCop is suitable for intact or degraded RNA, including FFPE samples (Appendix A, p.18).


The RiboCop V1.3 protocol has been optimized featuring less steps, reduced volumes for purification, and shorter incubation times compared to V1.2. Highly efficient rRNA depletion is maintained with no changes made to the Probe Mix, or to the Depletion steps (see Revision History, p.19). The provided RiboCop Kits still contain all components required for the V1.2 protocol, and full detailed and short procedures for V1.2 are included in this User Guide (p.14 - 17).

RiboCop is recommended for downstream NGS library preparation using the CORALL Total RNA-Seq Library Prep Kit (Cat. No.s 095, 096).

HYBRIDIZATION AND BEAD PREPARATION

45 min

10 min

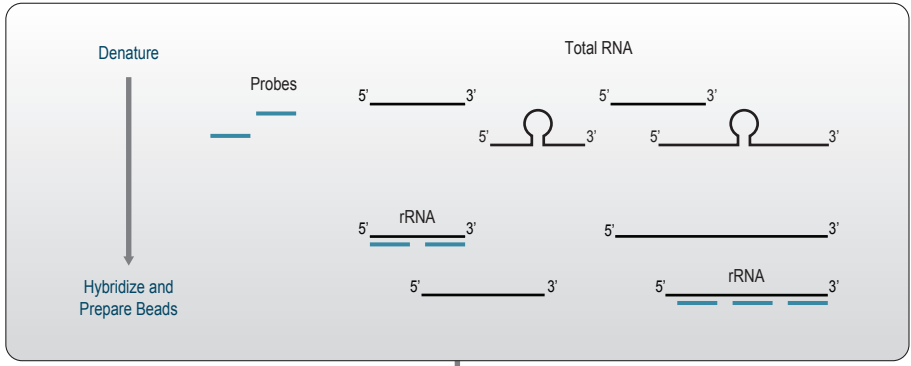

DEPLETION

45 min

20 min

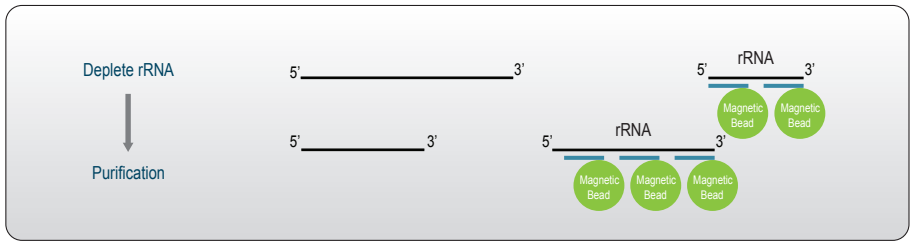


Figure 1. Schematic overview of the RiboCop V1.3 workflow. The overall workflow is identical to Ribocop V1.2, but with reduced timing for Bead Preparation and Final Purification.

2. Kit Components and Storage Conditions

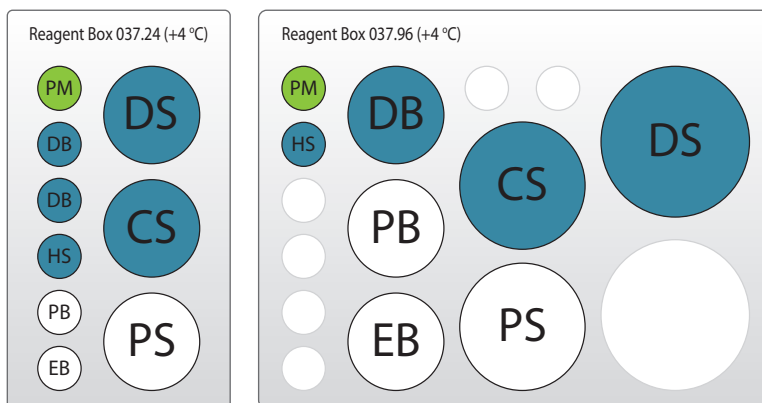


Figure 2. Location of kit components for 24 and 96 prep kits.

Kit Component	Tube Label	Volume* for		Storage
		24 preps	96 preps	
Hybridization Solution	HS ●	106 µl	423 µl	+4 °C
Probe Mix	PM ●	132 µl	528 µl	-20 °C/+4 °C
Depletion Beads	DB ●	1,980 µl	7,920 µl	+4 °C
Conditioning Solution	CS ●	3,960 µl	15,840 µl	+4 °C
Depletion Solution	DS ●	6,732 µl	26,928 µl	+4 °C
Purification Beads	PB ○	634 µl	2,535 µl	+4 °C
Purification Solution	PS ○	4,594 µl	18,375 µl	+4 °C
Elution Buffer	EB ○	1,109 µl	4,436 µl	-20 °C/+4 °C

* including ≥10% surplus

Upon receiving the RiboCop kit, store all components at +4 °C. **EB** ○ and **PM** ● can also be stored at -20 °C but avoid frequent freeze-thaw cycles. Before use, check the contents of **PS** ○ which may precipitate during shipping. If a precipitate is visible or the content appears milky, incubate at 37 °C until solution components dissolve completely. Equilibrate to room temperature again before use.

3. User-Supplied Consumables and Equipment

Check to ensure that you have all of the necessary materials and equipment before beginning rRNA depletion. All reagents, equipment and labware must be free of nucleases and nucleic acid contamination.

Reagents

- 80 % fresh ethanol (washing of Purification Beads, **PB** ○).

Equipment

- Magnetic rack or plate e.g., for 1.5 ml tubes: BcMag Magnetic separator-24, article# MS-03 from Bioclone; for 96-well plates: 96S Super Magnet Plate, article# A001322 from Alpaqua, or Dynamag™-96 Side/Side Skirted. Magnets, article # 12331D/12027 from Thermo Fisher.
- Benchtop centrifuge for spinning down liquids.
- Vortex mixer.
- Calibrated single-channel pipettes for handling 1 µl to 1,000 µl volumes.
- Thermomixer.
- UV-spectrophotometer to quantify RNA.

Labware,

- Suitable low-binding pipette tips (pipette tips with aerosol barriers recommended).
- 1.5 ml tubes, low binding, certified ribonuclease-free.
- 200 µl PCR tubes or 96-well plates and caps or sealing foil.
- Benchtop cooler or ice pellets in ice box (for short-term storage of RNA).

Optional Equipment and Solutions

- Automated microfluidic electrophoresis station (Agilent Technologies 2100 Bioanalyzer).
- Benchtop fluorometer and appropriate assays (for RNA quality control and quantification).
- Agarose gels, dyes, and electrophoresis rig (for RNA quality control).
- RNaseZap.
- RNase inhibitor.

The complete set of materials, reagents, and labware for quality control is not listed. Consult Appendix A (p.18) for more information.

4. Guidelines

RNA Handling

- RNases are ubiquitous, and special care should be taken throughout the procedure to avoid RNase contamination.
- Use commercial ribonuclease inhibitors (i.e., RNasin, Promega Corp.) to maintain RNA integrity when storing samples.
- Use a sterile and RNase-free workstation or laminar flow hood if available. Please note that RNases may still be present on sterile surfaces, and that autoclaving does not completely eliminate RNase contamination. Well before starting a library preparation, clean your work space, pipettes, and other equipment with RNase removal spray (such as RNaseZap, Ambion Inc.) as per the manufacturer's instructions. **ATTENTION:** Do not forget to rinse off any RNaseZap residue with RNase-free water after usage. Residues of RNaseZap may damage the RNA.
- Protect all reagents and your RNA samples from RNases on your skin by wearing a clean lab coat and fresh gloves. Change gloves after making contact with equipment or surfaces outside of the RNase-free zone.
- Avoid speaking above opened tubes. Keep reagents closed when not in use to avoid airborne RNase contamination.

Bead Handling

- Beads are stored at +4 °C and must be resuspended before usage. Beads can be resuspended by pipetting up and down several times or by vortexing. When properly resuspended, the solution should have a uniform brown color with no visible clumping on the walls or bottom of the tube or storage bottle.
- Beads may stick to certain pipette tips, in which case removing the beads from the inside of the tip may be impossible. Avoid resuspending by repeated pipetting and instead resuspend by vortexing if this occurs with your tips.
- Beads are superparamagnetic and are collected by placing the plate / tube in a magnetic plate or stand. The time required for complete separation will vary depending on the strength of your magnets, wall thickness of the wells / tubes, viscosity of the solution, and the proximity of the well / tube to the magnet. Separation time may need to be adjusted accordingly. When fully separated, the supernatant should be completely clear and the beads collected at one point or as a ring along the wall of the well / tube, depending on the magnet that was used.
- To remove the supernatant the plate / tube containing the beads has to stay in close contact with the magnet. Do not remove the plate / tube from the magnetic plate / stand when removing the supernatant, as the absence of the magnet will cause the beads to go into suspension again.

- When using a multichannel pipette to remove the supernatant, make sure not to disturb the beads. If beads were disturbed, ensure that no beads are stuck to the pipette tip opening and leave the multichannel pipette in the well for an extra 30 seconds before removing the supernatant. This way all beads can be recollected at the magnet and the clear supernatant can be removed.
- In general, beads should not be centrifuged during the protocol. However, should drops of fluid stay on the wall of the reaction tube / plate (e.g., after mixing by vortexing), centrifugation at 2,000 x g for 30 seconds should be carried out before placing the tube / plate on the magnetic stand / plate.
- Allowing the beads to dry out can damage them. Always keep the beads in suspension except for the short period after withdrawing the supernatant, and before adding the next reagent. Beads can be resuspended by vortexing, but make sure that beads are not deposited on the well / tube walls above the level of the liquid, where they can dry during incubation. If necessary, stuck beads can be collected by centrifuging the plate / tube briefly with a suitable benchtop centrifuge.

General

- The protocol can be performed in 1.5 ml tubes, PCR tubes, or PCR plates. When using PCR tubes or plates, shaking can be omitted and a thermocycler may be used.
- Pre-heat thermomixers (or thermocyclers) in advance of starting. Thermomixers may take several minutes to cool from 75 °C to 60 °C. To increase the speed of the protocol, use two thermomixers: set to 75 °C for step 4 and 60 °C for step 5.
- Mixing may be performed by pipetting, or gentle brief vortexing. Mix until the sample is homogeneous.
- Perform all pipetting steps with calibrated pipettes and always use fresh tips. Pipette carefully to avoid foaming as some solutions contain detergents.
- Equilibrate all necessary buffers at room temperature or as indicated in the preparation tables at the beginning of the protocol. Mix reagents well by vortexing or pipetting repeatedly and spin down briefly before use.
- Ensure that adequate volumes of all reagents and the necessary equipment are available and set to the proper temperatures before beginning the protocol.
- Unless explicitly mentioned, all steps should be carried out at room temperature (RT) between 20 °C and 25 °C. Results may be negatively impacted if the protocol is performed at temperatures outside this range. While reaction set-up is often performed at RT, incubation temperatures are explicitly defined and must be strictly adhered to.
- **PB** ○ and **PS** ○ are viscous solutions that require care to pipette accurately. Quickly spin down the tubes to collect all liquid at the bottom of the tube. Be sure to pipette slowly and check the graduation marks on your pipette tips when removing an aliquot.

5. Detailed Protocol RiboCop V1.3

Preparation

Hybridization	Bead Preparation and Depletion	Purification
HS ● } equilibrated PM ● } at RT	DB ● } equilibrated DS ● } at RT	PB ○ – stored at 4 °C PS ○ – stored at 4 °C 80 % EtOH – provided by user, prepare fresh! EB ○ – thawed at RT or stored at 4 °C
Thermomixer set to 75 °C / 1,250 rpm	Thermomixer set to 60 °C / 1,250 rpm	Equilibrate all reagents to room temperature for 30 minutes prior to use

Hybridization

Probe Mix (PM ●) and total RNA are mixed, denatured, and hybridized.

ATTENTION: Important notes for RiboCop Hybridization Steps:

- If a thermomixer is not available, input amounts ≤500 ng of total RNA can be processed in PCR tubes or plates and incubated in a thermocycler, without shaking.
- Bead Preparation (p.11) can be performed during the incubation at step 5.
- Place the Purification Beads (PB ○) and Purification Solution (PS ○) for step 16 at room temperature prior to starting the protocol, to ensure these have at least 30 minutes to equilibrate.

- 1 Prepare 1 - 1,000 ng of total RNA in a total volume of 26 µl. Dilute using RNase-free water if required.
- 2 Add 4 µl Hybridization Solution (HS ●).
- 3 Add 5 µl Probe Mix (PM ●) and mix thoroughly until homogeneous.
- 4 Denature samples using a thermomixer at 75 °C for 5 minutes with agitation at 1,250 rpm.
- 5 Decrease the temperature of the thermomixer to 60 °C and incubate the samples for 30 minutes with agitation at 1,250 rpm. **OPTIONAL:** Transfer the samples from step 4 to a second thermomixer set to 60 °C.

Bead Preparation

Depletion Beads (DB ●) must be prepared before use. These steps may be performed as a batch for up to 6 samples.

ATTENTION: Mix Depletion Beads (DB ●) fully before use.

- 6 Transfer 75 μ l Depletion Beads (DB ●) per reaction to a fresh tube.

- 7 Place the tube onto the magnet and let the beads collect for 2 - 5 minutes or until the supernatant is completely clear. Remove and discard the supernatant with a pipette while the tube remains in contact with the magnet.

- 8 Add 75 μ l Depletion Solution (DS ●) to the beads. Remove the tube from the magnet and resuspend the beads.

- 9 Place the tube back onto the magnet and let the beads collect for 2 - 5 minutes or until the supernatant is completely clear. Remove and discard the supernatant.

- 10 Repeat this washing step once (for a total of two washes).

- 11 Resuspend the beads in 30 μ l Depletion Solution (DS ●).

Depletion

Depletion Beads (DB ●) are used to remove the probe-hybridized ribosomal RNA.

ATTENTION: Avoid the formation of air bubbles while mixing.

- 12 Spin down the hybridized sample from step 5 and add 30 μ l of freshly prepared beads from step 11. Mix by pipetting up and down at least 8 times, or until homogeneous.

- 13 Put the sample back to the thermomixer and incubate at 60 °C for 15 minutes with agitation at 1,250 rpm.

- 14 Spin down briefly then place the sample on the magnet and let the beads collect for 5 minutes.

- 15 Recover and transfer 60 μ l of the supernatant containing the rRNA-depleted RNA to a fresh tube. Avoid disturbing the collected beads to prevent rRNA contamination.
ATTENTION: Do not throw away the supernatant.

Purification

The depleted RNA is purified using magnetic beads. The purification reagents (**PB** ○, **PS** ○, and **EB** ○) should equilibrate for 30 minutes at room temperature before use. The Purification Beads (**PB** ○) must be fully resuspended before use. Thorough mixing by pipetting or vortexing is recommended.

- 16 Add 24 μ l Purification Beads (**PB** ○) and 108 μ l Purification Solution (**PS** ○) to the supernatant. Mix well by pipetting. Incubate for 5 minutes at room temperature.

- 17 Place the sample onto a magnet and let the beads collect for 5 - 10 minutes or until the supernatant is completely clear. **NOTE:** The speed of bead collection depends on the strength of the magnet.

- 18 Remove and discard the clear supernatant without removing the sample from the magnet. Make sure that accumulated beads are not disturbed.


- 19 Add 120 μ l of 80 % EtOH and incubate the beads for 30 seconds. Leave the sample on the magnet as beads should not be resuspended during this washing step. Remove and discard the supernatant. **ATTENTION:** When using 1.5 ml tubes use 150 μ l of 80 % EtOH to ensure beads are fully covered by EtOH.

- 20 Repeat this washing step once for a total of two washes. Make sure the supernatant is removed completely.

- 21 Leave the sample in contact with the magnet and let the beads dry for 5-10 minutes or until all ethanol has evaporated. **ATTENTION:** Dry the beads at room temperature only and do not let the beads dry too long (visible cracks appear), this will negatively influence the elution and the resulting library yield.

- 22 Add 12 μ l of Elution Buffer (**EB** ○), remove the sample from the magnet and resuspend the beads properly in **EB** ○. Incubate for 2 minutes at room temperature.

- 23 Place the sample onto the magnet and let the beads collect for 2 - 5 minutes or until the supernatant is completely clear.

- 24 Transfer 10 μ l of the supernatant into a fresh tube. Depleted RNA is now ready for quality control and downstream use (e.g., for NGS library preparation).  Safe stopping point. RNA can be stored at ≤ -20 °C at this point.

6. Short Procedure RiboCop V1.3

ATTENTION: Spin down solutions before opening tubes or plates!

45 min

Hybridization and Bead Preparation

Hybridization

- Prepare 1 - 1,000 ng total RNA in 26 μ l.
- Add 4 μ l **HS** ●.
- Add 5 μ l **PM** ●, mix until homogeneous.
- Denature for 5 min at 75 °C / 1,250 rpm.
- Incubate for 30 min at 60 °C / 1,250 rpm.

Bead Washing

- Resuspend **DB** ●, transfer 75 μ l to a fresh tube.
- Place on magnet for 2 - 5 min, discard supernatant.
- Resuspend beads in 75 μ l **DS** ●, incubate 2 min on magnet, discard supernatant. Repeat once.
- Resuspend beads in 30 μ l **DS** ●.

45 min

Depletion and Purification

Depletion

- Spin down hybridized sample. Add 30 μ l of prepared beads. Mix by pipetting 8x, or until homogeneous.
- Incubate for 15 min at 60 °C / 1,250 rpm. Spin down.
- Place on magnet for 5 min.
- Transfer 60 μ l supernatant to a fresh tube. **ATTENTION:** The supernatant contains the rRNA depleted RNA.

Purification

- Add 24 μ l **PB** ○ and 108 μ l **PS** ○, mix well, incubate for 5 min at RT.
- Place on magnet for 5 - 10 min, discard supernatant.
- Wash the beads twice with 120 - 150 μ l 80 % EtOH, 30 sec. **ATTENTION:** Use 150 μ l for 1.5 ml tubes.
- Air dry beads for 5 - 10 min. **ATTENTION:** do not over dry the beads!
- Add 12 μ l **EB** ○, remove from magnet, mix well, incubate 2 min at RT.
- Place on magnet for 2 - 5 min, transfer 10 μ l of the supernatant to a fresh tube. 📌 Safe stopping point.

7. Detailed Protocol RiboCop V1.2

Preparation

Hybridization	Bead Conditioning and Depletion	Purification
HS ● } equilibrated PM ● } at RT	DB ● } equilibrated CS ● } at RT DS ● }	PB ○ – stored at 4 °C PS ○ – stored at 4 °C 80 % EtOH – provided by user, prepare fresh! EB ○ – thawed at RT or stored at 4 °C
Thermomixer set to 75 °C	Thermomixer set to 60 °C	Equilibrate all reagents to room temperature for 30 minutes prior to use

Hybridization

Probe Mix (PM ●) and total RNA are mixed, denatured, and hybridized.

ATTENTION: Important notes for RiboCop Hybridisation Steps:

- Bead Conditioning (p.15) is performed during the incubation at step 5.
- Place the Purification Beads (PB ○) and Purification Solution (PS ○) for step 17 at room temperature prior to starting the protocol, to ensure these have at least 30 minutes to equilibrate.

- 1 Prepare 1 - 1,000 ng of total RNA in a total volume of 26 µl. Dilute using RNase-free water if required.
- 2 Add 4 µl Hybridization Solution (HS ●).
- 3 Add 5 µl Probe Mix (PM ●) and vortex gently.
- 4 Denature samples using a thermomixer at 75 °C for 5 minutes with gentle agitation at 400 rpm.
- 5 Decrease the temperature of the thermomixer to 60 °C and incubate the samples for 30 minutes with agitation at 400 rpm. **OPTIONAL:** Transfer the samples from step 4 to a second thermomixer set to 60 °C.

Bead Conditioning

Depletion Beads (**DB ●**) must be conditioned before use.

- 6 Mix Depletion Beads (**DB ●**) properly. Transfer 75 μ l per reaction to a fresh tube.

- 7 Place the tube in a magnetic rack and let the beads collect for 2 - 5 minutes or until the supernatant is completely clear (depends on the magnet strength). Remove and discard the supernatant with a pipette while the tube remains in contact with the magnet.

- 8 Add 75 μ l Conditioning Solution (**CS ●**) per reaction. Remove the tube from the magnetic rack and resuspend the beads, then transfer the tube back to the magnetic rack. Incubate for 2 minutes. Remove and discard the supernatant.

- 9 Repeat this conditioning step once (for a total of two rounds of conditioning).

- 10 Add 75 μ l Depletion Solution (**DS ●**). Remove the tube from the magnetic rack and resuspend the beads. Transfer the tube to the magnetic rack and let the beads collect for 2 - 5 minutes or until the supernatant is completely clear. Remove and discard the supernatant.

- 11 Repeat this washing step twice (for a total of three washes).

- 12 Resuspend the beads in 30 μ l Depletion Solution (**DS ●**).

Depletion

Depletion Beads (**DB ●**) are used to remove the probe-hybridized ribosomal RNA.

- 13 Spin down hybridized sample as soon as incubation (step 5) is finished. Add 30 μ l freshly conditioned beads from step 12. Mix by pipetting up and down at least 8 times. **REMARK:** Set pipette to a larger value for mixing but avoid formation of air bubbles.

- 14 Put the tube back to the thermomixer and incubate at 60 °C for 15 minutes with gentle agitation at 400 rpm. Spin down.

- 15 Place the tube in a magnetic rack and let the beads collect for 5 minutes.

- 16 Recover and transfer 60 μ l of the supernatant containing the rRNA-depleted RNA to a fresh tube. Avoid disturbing the collected beads to prevent rRNA contamination. **ATTENTION:** Do not throw away the supernatant.

Purification

The depleted RNA is purified using magnetic beads. The Purification Beads (**PB** ○) and Purification Solution (**PS** ○) should equilibrate for 30 minutes at room temperature before use. **PB** ○ may have settled and must be properly resuspended before adding them to the reaction.

- 17 Add 24 μ l Purification Beads (**PB** ○) and 108 μ l Purification Solution (**PS** ○) to the supernatant. Mix well by pipetting. Incubate for 20 minutes at room temperature.

- 18 Place the tube onto a magnetic rack and let the beads collect for 5 - 10 minutes or until the supernatant is completely clear. **REMARK:** The speed of bead collection depends on the strength of the magnet.

- 19 Remove and discard the clear supernatant without removing the tube from the magnetic rack. Make sure that accumulated beads are not disturbed.

- 20 Add 30 μ l of Elution Buffer (**EB** ○), remove the tube from the magnet and resuspend the beads properly in **EB** ○. Incubate for 2 minutes at room temperature.

- 21 Add 66 μ l of Purification Solution (**PS** ○) to the beads / **EB** mix to re-precipitate the sample. Mix thoroughly and incubate for 5 minutes at room temperature.

- 22 Place the tube onto a magnetic rack and let the beads collect for 2 - 5 minutes.

- 23 Remove and discard the clear supernatant without removing the tube from the magnetic rack. Make sure that accumulated beads are not disturbed.


- 24 Add 120 μ l of 80 % EtOH and incubate the beads for 30 seconds. Leave the tube in contact with the magnet as beads should not be resuspended during this washing step. Remove and discard the supernatant. **ATTENTION:** When using 1.5 ml tubes use 150 μ l of 80 % EtOH to ensure beads are fully covered in EtOH.

- 25 Repeat this washing step once for a total of two washes. Make sure the supernatant is removed completely.

- 26 Leave the tube in contact with the magnet and let the beads dry for 5 -10 minutes or until all ethanol has evaporated. **ATTENTION:** Dry the beads at room temperature only and do not let the beads dry too long (visible cracks appear), this will negatively influence the elution and the resulting library yield.

- 27 Add 12 μ l of Elution Buffer (**EB** ○), remove the tube from the magnet and resuspend the beads properly in **EB** ○. Incubate for 2 minutes at room temperature.

- 28 Place the tube onto a magnetic rack and let the beads collect for 2 - 5 minutes or until the supernatant is completely clear.

- 29 Transfer 10 μ l of the supernatant into a fresh tube.  Safe stopping point. RNA can be stored at ≤ -20 °C at this point.

8. Short Procedure RiboCop V1.2

ATTENTION: Spin down solutions before opening tubes or plates!

45 min

Hybridization and Bead Conditioning

Hybridization

- Prepare 1 - 1,000 ng total RNA in 26 μ l.
- Add 4 μ l **HS** ●.
- Add 5 μ l **PM** ●, mix until homogeneous.
- Denature for 5 min at 75 °C / 400 rpm.
- Incubate for 30 min at 60 °C / 400 rpm.

Bead Conditioning

- Resuspend **DB** ●, transfer 75 μ l to a fresh tube.
- Place on magnet for 2 - 5 min, discard supernatant.
- Resuspend beads in 75 μ l **CS** ●, incubate 2 min on magnet, discard supernatant. Repeat once.
- Resuspend beads in 75 μ l **DS** ●, place on magnet for 2 - 5 min, discard supernatant. Repeat twice.
- Resuspend beads in 30 μ l **DS** ●.

75 min

Depletion and Purification

Depletion

- Spin down hybridized sample. Add 30 μ l conditioned beads. Mix by pipetting 8x, or until homogeneous.
- Incubate for 15 min at 60 °C / 400 rpm. Spin down.
- Place on magnet for 5 min.
- Transfer 60 μ l supernatant to a fresh tube. **ATTENTION:** The supernatant contains the rRNA depleted RNA.

Purification

- Add 24 μ l **PB** ○ and 108 μ l **PS** ○, mix well, incubate for 20 min at RT.
- Place on magnet for 5 - 10 min, discard supernatant.
- Add 30 μ l **EB** ○, remove from magnet, mix well, incubate 2 min at RT.
- Add 66 μ l **PS** ○, mix well, incubate 5 min at RT.
- Place on magnet for 2 - 5 min, discard supernatant.
- Wash the beads twice with 120 - 150 μ l 80 % EtOH, 30 sec.
- Air dry beads for 5 - 10 min. **ATTENTION:** do not over dry the beads!
- Add 12 μ l **EB** ○, remove from magnet, mix well, incubate 2 min at RT.
- Place on magnet for 2 - 5 min, transfer 10 μ l of the supernatant to a fresh tube.

9. Appendix A: RNA Requirements and Results

Potential Contaminants

RNA samples should be free of salts, metal ions, and organic solvents, which can be carried over from RNA extraction. Several sources of contamination (e.g., proteins, chaotropic salts, and phenol) can be detected with a UV-Vis spectrophotometer. An acceptably pure RNA sample should have an A260/A280 ratio between 1.8 and 2.1. The A260/A230 ratio should also be greater than 1.8. Contaminants may have a negative impact on the efficiency of the protocol. For isolation of high quality total RNA we recommend Lexogen's SPLIT RNA Extraction Kit (Cat. No. 008.48).

RNA Input Amount and Quality

The recommended input range for RiboCop is 1 - 1,000 ng of total RNA. RiboCop is suitable for intact or degraded RNA, including Formalin Fixed Paraffin-Embedded (FFPE) samples. FFPE RNA should best be treated with DNase prior to ribo-depletion with RiboCop. Recommended input for DNase treatment is ≥ 50 ng of FFPE total RNA. Spike-in controls, including Lexogen's Spike-In RNA Variant Controls (SIRVs, Cat. No.s 025, 050, 051), should be added to the RNA sample before RiboCop (or prior to DNase treatment for FFPE samples). The spike-in amount must be calculated relative to the target RNA fraction (e.g., ribo-depleted RNA). We recommend targeting 0.1 - 0.2 % of SIRV-mapped reads for FFPE samples, or 1% for higher quality samples. For assistance with SIRV spike-in calculation, please contact support@lexogen.com.

Typical Results

Quality control of depleted RNA (using microcapillary electrophoresis, e.g., Bioanalyzer PicoChip, Agilent Technologies) is recommended prior to conducting library preparation and sequencing runs. Successful rRNA depletion results in removal of 28S and 18S rRNA peaks. These rRNA peaks usually dominate electropherograms of intact total RNA and should be absent after RiboCop depletion as shown in Figure 3.

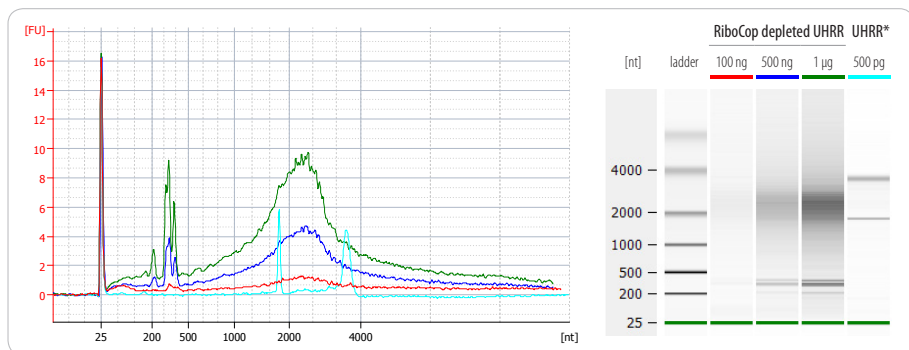


Figure 3. Results of RiboCop V1.3 ribo-depletion. Universal Human Reference RNA (UHRR) was used as input for RiboCop V1.3 with different total RNA input amounts (100 ng red, 500 ng dark blue, 1 µg green). * Undepleted UHRR (Cyan: 500 pg) showing 28S and 18S rRNA peaks.

10. Appendix B: Downstream Processing

This protocol was tested extensively with Universal Human Reference RNA (UHRR) and Human Brain Reference RNA (HBRR) as well as mouse and rat samples. Depleted RNA samples are ideally suited for downstream NGS library preparation using Lexogen's CORALL Total RNA-Seq Library Prep Kit (Cat. No. 095, 096). Up to 10 µl of the eluted rRNA-depleted RNA may be used as input for CORALL library preparation.

11. Appendix C: Revision History

Publication No. / Revision Date	Change	Page
037UG073V0300 Sep. 9, 2019	V1.3 protocol added: faster workflow, no change to kit components, V1.2 protocol remains optional.	10 - 17
	V1.3: Shaking speed increased to 1,250 rpm in steps 4, 5, and 12.	10 - 11
	V1.3: Removal of CS bead conditioning steps.	11
	V1.3: Reduction from three DS washes to two washes.	11
	V1.3: PB + PS binding time reduced to 5 min at step 16.	12
	V1.3: Removal of double bind steps (EB and PS).	12
	V1.3: Use 150 µl of 80 % EtOH in step 24 when using 1.5 ml tubes.	12
	V1.3 Short Procedure updated and reformatted.	13
	V1.2 Detailed Protocol and Short Procedure moved.	14 - 16
037UG073V0201 Jul. 26, 2017	Consistency changes.	
	Added Attention note to step 16.	10
037UG073V0200 Aug. 19, 2016	Released RiboCop V1.2.	
	Lowered input amount to 1 ng.	5
	Introduction of Hybridization Solution (HS) in step 2.	5
	Adjusted rpm-values.	9
	Adjusted reaction volumes in step 16, 17, 27.	10, 11
037UG073V0104 Mar. 29, 2016	Lowered input amount to 10 ng.	4, 9, 12
037UG073V0100 Nov. 10, 2015	Initial Release.	

Associated Products:

022 (Purification Module with Magnetic Beads)

025, 050, 051 (SIRVs Spike-in RNA Variant Control Mixes)

095 (CORALL Total RNA-Seq Library Prep Kit)

RiboCop rRNA Depletion Kit V1.3 · User Guide

Lexogen GmbH

Campus Vienna Biocenter 5

1030 Vienna, Austria

Telephone: +43 (0) 1 345 1212-41

Fax: +43 (0) 1 345 1212-99

E-mail: support@lexogen.com

© Lexogen GmbH, 2019

Lexogen, Inc.

51 Autumn Pond Park

Greenland, NH 03840, USA

Telephone: +1-603-431-4300

Fax: +1-603-431-4333

www.lexogen.com